

1 **Fully Automatic In-Syringe Magnetic Stirring-Assisted Dispersive Liquid-Liquid**
2 **Microextraction hyphenated to High Temperature Torch Integrated Sample**
3 **Introduction System-Inductively Coupled Plasma Spectrometer with Direct**
4 **Injection of the Organic Phase**

5
6 **Raquel Sánchez,¹ Burkhard Horstkotte,^{2,3} Kateřina Fikarová,² Hana Sklenářová,²**
7 **Salvador Maestre,¹ Manuel Miró,^{2,3*} Jose-Luis Todolí^{1*}**

8
9 ¹ University of Alicante, Department of Analytical Chemistry, Nutrition and Food
10 Sciences, P.O. Box 99, 03080, Alicante, Spain

11 *Corresponding author. E-mail: jose.todoli@ua.es

12
13 ² Charles University, Department of Analytical Chemistry, Faculty of Pharmacy,
14 Heyrovského 1203, 500 05 Hradec Králové, Czech Republic

15
16 ³ FI-TRACE group, University of the Balearic Islands, Department of Chemistry,
17 Carreterra de Valldemossa km 7.5, 07122 Palma de Mallorca, Spain

18 *Corresponding author. E-mail: manuel.miro@uib.es

19

20

21 **Abstract**

22 A proof of concept study involving the on-line coupling of automatic dispersive liquid-liquid
23 microextraction (DLLME) to ICP OES with direct introduction and analysis of the organic
24 extract is herein reported for the first time. The flow-based analyzer features a Lab-In-Syringe
25 (LIS) setup with an integrated stirring system, a Meinhard[®] nebulizer in combination with a
26 heated single-pass spray chamber, and a rotary injection valve, used as on-line interface
27 between the microextraction system and the detection instrument. Air segmented flow was used
28 for delivery of a microliter fraction of the non-water miscible extraction solvent, 12 μ L of
29 xylene, to the nebulizer. All sample preparative steps including magnetic stirring assisted
30 DLLME were carried out inside the syringe void volume as a size-adaptable yet sealed mixing
31 and extraction chamber. Determination of trace level concentrations of cadmium, copper, lead,
32 and silver as model analytes has been demonstrated by microextraction as
33 diethyldithiophosphate (DDTP) complexes. The automatic LIS-DLLME method features
34 quantitative metal extraction, even in troublesome sample matrices, such as seawater, salt, and
35 fruit juices, with relative recoveries within the range of 94-103%, 93-100% and 92-99%,
36 respectively. Furthermore, no statistically significant differences at the 0.05 significance level
37 were found between concentration values experimentally obtained and the certified values of
38 two serum standard reference materials.

39

40

41

42

43

44

45

46

47 Inductively coupled plasma (ICP)-based techniques are deemed the most universal atomic
48 spectrometric techniques for metal assays as they enable detection of practically all metals and
49 metalloids of the periodic table with excellent sensitivity, reproducibility and sample
50 throughput. Besides, continuous improvements of instrumentation and software make ICP-
51 based techniques user-friendly for routine analysis. However, limitations of instrumental
52 robustness and background interferences in the analysis of high salt content solutions or samples
53 with elevated organic load might jeopardize the reliability of the analytical method. In fact, the
54 occurrence of this kind of matrices might deteriorate the nebulization efficiency, plasma
55 electron density, and even lead to plasma torch shutdown. The sensitivity of ICP OES and ICP-
56 MS based methods does not in some instances suffice for the detection of elements at trace
57 level concentrations, as might be the case in environmental surveillance studies or health
58 risk/exposure assessment. Several approaches have been developed to overcome or minimize
59 these drawbacks, including sorbent-based analyte preconcentration,¹⁻³ the addition of oxygen to
60 avoid carbon deposition, or the elimination of the sample matrix by electrothermal sample
61 vaporization prior to sample injection into the plasma.^{4,5}

62 With regard to sample handling strategies, liquid-liquid extraction (LLE) of hydrophobic metal
63 or oxyanion complexes has proven to be a powerful pre-concentration and clean-up approach
64 for trace metal analysis by graphite furnace (GFAAS) and flame atomic adsorption
65 spectrometry.^{6,7} In contrast, measurements by ICP-based techniques require generally in-line
66 desolvation, solvent emulsification, or solvent dilution to yield steady nebulization conditions.^{4,5}
67 Few papers report on LLE with back-extraction of the target species into an aqueous phase as a
68 front end to ICP detection.⁸⁻¹¹ This approach combines the advantages of LLE including salt
69 removal and avoiding typical problems of on-line SPE (backpressure, filter blockage, etc.) along
70 with eluate compatibility with the detector. However, both the operational time and, if
71 automated, the instrumental complexity and effort, e.g. to yield reproducible solvent
72 introduction and reliable phase separation, refrained this LLE mode from further
73 development.^{1,12,13}

74 As an alternative to matrix elimination, the use of a high efficiency micronebulizer in
75 combination with a heated spray chamber, termed high temperature torch integrated sample
76 introduction system (h-TISIS), has been reported for reliable ICP- assays of complex
77 samples.^{14,15} With the injection of a mere few microliters of sample, matrix effects have showed
78 to become insignificant as the temperature of the spray chamber is set at 350°C for fuels and
79 diverse acid digested environmental samples.^{14,15} Moreover, direct analysis of hydrocarbon
80 samples has also proven to be feasible.¹⁴ Readers are referred to a series of reviews describing
81 instrumental aspects and successful applications of this approach for metal/metalloid
82 determination in organic matrices.^{4,5}

83 This work was sparked by the consideration that such versatile sample introduction system
84 could be hyphenated to automatic liquid-liquid microextraction for expedient analysis of
85 organic extracts. In this context, the Lab-In-Syringe (LIS) concept^{16,17} has gained considerable
86 attention as a sample handling tool for straightforward and versatile batch-wise automation of
87 liquid-phase based approaches. Taken as a sequel of the second generation of flow analysis, also
88 called sequential injection analysis,^{18,19} LIS is featured by carrying out the entire procedure in
89 the void volume of the barrel of a gas-tight automated syringe pump operating as an enclosed
90 mixing chamber. Of special impact is the integration of a magnetic stirring bar into the syringe
91 for homogenous sample/reagent mixture and solvent dispersion.^{20,21}

92 While there has been significant work harnessing flow-based approaches (mostly flow injection
93 and sequential injection) for automated liquid-liquid extraction of metal species,^{6,7,22-25} with
94 potential implementation in microfluidic devices,^{24,26,27} prior to on-line atomic spectrometric
95 detection, reviewed elsewhere,^{3,28,30} just few papers report on employing LIS, whose versatility
96 has not been fully explored yet. LIS for metal assays has been merely coupled to atomic
97 absorption spectrometric measurements, *namely*, mercury microextraction and cold vapor
98 atomic absorption spectroscopy (AAS)^{31,32} and more recently to non-dispersive liquid phase
99 extraction of silver followed by GFAAS,³³ yet studies concerning on-line dispersive liquid-

100 liquid microextraction (DLLME) as a front-end microextraction approach to multi-elemental
101 ICP OES/MS are still missing.

102 In this paper, in-syringe DLLME is explored for the first time as a “front-end” versatile
103 microextraction platform for ICP-based detection. Diethyldithiophosphate (DDTP) is used as a
104 selective chelating reagent on the basis of its ability of complexing metal species at the usual
105 acidic pH values for sample conservation³⁴ as opposed to its carbamate counterparts, i.e. no
106 additional buffering of sample is needed, which, in turn, make the analytical method
107 straightforward (with no need of pH optimization) and less prone to blank contamination. As a
108 consequence of the high stability constants of the DDTP chelates, even in strong acidic
109 conditions, back-extraction methods with increasing of the acidity and/or the addition of
110 competing metal species are proven inappropriate for quantitative recovery of DDTP complexed
111 metals.^{35,36} To tackle this issue, we have exploited h-TISIS as a viable interface for the direct
112 injection of the metal containing organic extracts into the ICP system. With this interface,
113 organic matrices are permitted whereby analyte dilution in the back-extraction solution in
114 conventional liquid-phase microextraction approaches of trace metals is circumvented.
115 Cadmium, copper, lead, and silver were chosen as model analytes and analyzed in varied
116 environmental and food matrices.

117

118 **Material and methods**

119 *Chemicals and samples*

120 Ultrapure water was supplied by a three-step ion-exchange system Milli-Q, fed by reverse
121 osmosis, Elix 3, both from Millipore (El Paso, TX, USA). Isopropanol and xylene (Panreac
122 Química S.A., Barcelona, Spain) were employed for the cleaning of the syringe barrel and flow
123 system prior to each extraction and as extraction solvent, respectively. Diethyldithiophosphate
124 ammonium salt (DDTP, 95 %) was obtained from Sigma Aldrich (Saint Quentin Fallavier,
125 France) and used as a chelating reagent, prepared in aqueous medium. 65% HNO₃ (Suprapur®,
126 Merck KGaA, Darmstadt, Germany) was used to prepare washing solutions and acidify the

127 standards and samples. An ICP multielement standard solution (Merck IV, Merck KGaA,
128 Darmstadt, Germany) containing 1000 mg element per litre was used to prepare the standards
129 by serial dilutions. Stock and standard solutions were prepared in 2 % (v/v) HNO₃. Organic
130 multielement standards were prepared by dissolving a certified material (Conostan[®] S-21,
131 Conoco Specialty Products, Inc., Ponca City, Oklahoma, USA) in xylene. In order to evaluate
132 the reliability of the automatic system for handling complex matrices, a variety of real samples
133 were analyzed: seawater, salt, salt without sodium, grape juice and apple juice. Salt and juice
134 samples were bought in a local supermarket. Coastal seawater was collected in Alicante using
135 pre-cleaned polyethylene flasks. The sample was taken at an approximately 50 cm depth and
136 stored at 4°C in the laboratory. Salt samples were prepared by dissolving 3.5 g of salt in 10 mL
137 of Milli-Q water. All samples were filtered using 0.45 µm nylon syringe filters (Filter-Lab[®],
138 Filtros Anovia, Barcelona, Spain). Two certified lyophilized control serum samples (ClinChek[®]
139 Controls, Recipe[®], Munich, Germany) were used as quality control (QC) materials for
140 evaluation of the trueness of the analytical method. Serum samples were reconstituted in 3.0 mL
141 of ultrapure water with gentle mixing until complete dissolution of the lyophilised material.

142

143 *Flow setup for automated DLLME*

144 The system configuration for lab-in-syringe dispersive liquid-liquid microextraction (LIS-
145 DLLME)-ICP OES assays is illustrated in Fig. 1 and a close up is presented in Fig S1. In all
146 experiments, a MicroSIA device from FIALab Instruments Inc. (Seattle, WA) was used to
147 assemble the flow manifold. It integrates a 30 mm Stroke OEM low pressure Syringe Pump (SP,
148 Cavro XCalibur) and an 8 port selection valve (SV, Vici Valvo) furnished with a PTFE rotor.
149 The MicroSIA system contains two auxiliary supply ports of 5 and 24 V herein utilized for
150 stirring activation and ICP triggering. The SP is furnished with a rotary head valve (HV) with
151 three selectable ports (IN, OUT, and TOP) for tubing connections. A 5 mL-glass syringe (30
152 mm lift, 1.45 mm id, Tecan) was used for performing all solution handling including the
153 DLLME procedure inside. A commercial PTFE covered magnetic stirring bar of 14 mm size

154 (4.5 mm diameter) was placed in the syringe barrel. To diminish the resulting dead volume at
155 syringe emptying, the stirrer was flattened by sand papering to 3.5 mm height and made to
156 length in order to fit snugly into the syringe. The stirrer was forced to spin at approximately 800
157 rpm by generating a rotating magnetic field outside the syringe (see Fig. 1 and Fig. S1). To this
158 end, a pile of seven neodymium magnets (each 3 mm x 5 mm Ø) was hot-glued on top of a
159 commercial cooling ventilator (12 VDC supply) serving as a cost-effective brushless motor
160 (wings and protection removed). The motor was connected to the syringe piston bar so that the
161 magnets were leveled with the stirring bar inside the syringe at any time. The motor was
162 powered by the 5 V supply port of the MicroSIA and activated (generating a rotating magnetic
163 field) by software control. By careful adjustment of this arrangement, stirring velocities
164 exceeding 800 rpm were proven applicable

165 Lateral ports 2-6 of the SV (see Fig. 1) were connected to 2 % (v/v) HNO₃ (2), isopropanol (3)
166 and 15 % (v/v) HNO₃ (8) for syringe chamber cleaning; extraction solvent (4), sample (5), and
167 complexing reagent (6). Using a very short tube of PEEK piercing a wider silicone tube for
168 drainage, port 1 allowed both syringe content discharge to waste during cleaning but also
169 aspiration of air (see Fig. 1). Air inside the syringe enabled vortex formation by stirring, thus
170 promoting solvent dispersion.

171 Port IN on the syringe HV was connected to the central port of the SV via a 15 cm long holding
172 coil (HC, PTFE tube, 1.0 mm i.d.). Port OUT was used to empty the syringe to waste without
173 passing the HC. The TOP position was connected via a 20 cm transfer line (0.5 mm i.d.) to a
174 low pressure (PEEK stator and rotor) six-port injection valve (IV) from Vici-Valco (Schenkon,
175 Switzerland), used as interface between the LIS-based microextraction system and the ICP
176 OES. A PEEK capillary of 8 cm (0.25 mm i.d.) was used as injection loop, the total injection
177 volume including the valve rotor channel was estimated as 12 µL.

178 Instrumental control of the extraction system was done via USB using the open-source software
179 Cocosoft, version 4.3 (FI-TRACE, University of the Balearic Islands).³⁷ The software is written
180 in Python programming language and enables the use of variables, loops, routines, and

181 conditionals, and communication via serial interface. Triggering of ICP OES activation and data
182 registration was done by relay contact using the 24 V supply port of the MicroSIA instrument.

183

184 *ICP OES measurements*

185 An Optima 4300 DV Perkin-Elmer ICP OES spectrometer (Uberlingen, Germany) was used as
186 detection instrument and the emission intensity signals were axially taken. The system was
187 equipped with a 40.68 MHz free-running generator and a polychromator with an echelle grating.
188 Table 1 summarizes the operational instrumental conditions.

189 A glass concentric nebulizer (TR-50-C3, Meinhard®, Golden, CA) was fitted to a 12 cm³ glass
190 single pass spray chamber (h-TISIS).³⁸ The h-TISIS was jacketed with a copper coil connected
191 to a power supply so as to heating the chamber at will. Hereto, the coil temperature was
192 programmed by means of a thermocouple attached to its surface (Desin Instruments, Barcelona,
193 Spain).¹⁴

194 The solutions were delivered to the nebulizer by a peristaltic pump (Gilson Minipuls3 Model
195 M312, Villiers-le-Bel, France) and a 0.19-mm i.d. PVC-based material with plasticizer (Tygon®
196 R-3607, Ismatec, S.A.) tubing was employed.

197 An air-segmented flow injection methodology was selected to deliver sample volumes at the 5-
198 15 µL level to the instrument. Air was continuously aspirated by means of a peristaltic pump. At
199 a given time and precisely controlled by software, a sample plug was driven to the nebulizer
200 using a carrier stream of air to avoid sample dispersion. Images of the injection of the analyte-
201 containing organic phase into the ICP torch are compiled in Fig S2. With this system, oxygen
202 was not needed to minimize background interferences in troublesome samples because of two
203 facts: (i) the injected sample volume was a mere of a few microliters; and, (ii) the oxygen in the
204 air stream continuously aspirated could boost the total carbon combustion. Therefore, negligible
205 soot deposits were found throughout the present work.

206

207

208 *Analytical protocol*

209 The analytical workflows are given as supplementary materials (Tables S1 and S2). The
210 DLLME protocol was started by cleaning the syringe with (1) isopropanol to remove any
211 residues of the extraction solvent from the previous extraction, (2) 15% (v/v) HNO₃ and two
212 times with 2% (v/v) HNO₃ to keep the syringe free from metal traces, and (3) with the
213 corresponding sample solution, that is, 2%(v/v) HNO₃ for blank measurements or the sample
214 solution itself from position 5 of the SV.

215 The in-syringe DLLME protocol is performed as follows: 250 μL of air (to promote vortex
216 formation with the consequent solvent dispersion), 270 μL of xylene, 3600 μL of sample, a 20
217 μL air plug (to avoid contact between sample and chelating reagent in the HC), 250 μL of
218 reagent solution, and a final volume of 180 μL air to empty the overall HC content into the
219 syringe barrel were sequentially aspirated. Immediately before the aspiration of the extraction
220 solvent, stirring at 800 rpm was activated. After an extraction time of 120 s, the stirring was
221 deactivated for phase separation for 30 s, which allowed the xylene droplets to float and to
222 coalesce. Eight repeated activations of the stirrer for a minimum time (< 1 s, not achieving the
223 final stirring rate) were done to remove any xylene residues, which were stuck on the stirring
224 bar.

225 In the final step, the organic phase was pushed at 80 μL s⁻¹ towards the injection valve first to
226 clean the transfer line and push out any residues from the previous injection to waste. Then,
227 aliquots of the solvent (12 μL) were injected repeatedly into ICP OES by IV activation into the
228 air flow carrying the injected volume to the h-TISIS at a delivery flow rate of 50 μL min⁻¹.
229 Every organic extract was injected three times for assessing the repeatability of the ICP
230 readouts. Finally, the aqueous syringe content was emptied to waste with the HV in position
231 OUT.

232

233

234

235 **Results and Discussion**

236 *Investigation of the h-TISIS-ICP OES operational conditions*

237 Parameters related to the nebulization and ICP OES measurements including the injection
238 volume of the organic phase, the nebulizer gas flow rate and the spray chamber temperature
239 were evaluated. For injection volumes of xylene larger $> 12 \mu\text{L}$, the plasma was unstable and
240 tended to shut down. The nebulizer gas flow rate was also optimized. The evaluated values were
241 in the range of $0.15\text{-}0.40 \text{ L min}^{-1}$. It was verified that the optimum nebulizer gas flow rate in
242 terms of sensitivity was 0.26 L min^{-1} . Higher flow rates might not ensure the quantitative
243 evaporation of the solvent in the aerosol phase within the spray chamber because of the short
244 residence times but lower flow rates might lead to excessively big aerosol droplets.

245 The effect of the evaporation chamber temperature on the analytical performance was also
246 investigated. ICP OES signal intensities for Ag, Cd, Cu and Pb were thus recorded at h-TISIS
247 temperatures ranging from 150 to $400 \text{ }^\circ\text{C}$. The h-TISIS spray chamber working at temperatures
248 $> 300^\circ\text{C}$ provided 8, 7 and 12 fold-peak height improvements with respect to those at room
249 temperature for Ag, Cd, Cu and Pb, respectively (see Fig. 2). This was due to the enhancement
250 of the aerosol solvent evaporation inside the chamber and, hence, of the analyte mass delivered
251 to the plasma. The working temperature was set to 350°C because, under these circumstances,
252 non-spectral interferences by the solvent itself were practically negligible.^{14,15}

253 The signal obtained for organic standards with h-TISIS working at the optimum experimental
254 conditions was compared with a conventional introduction system (*i.e.*, cyclonic spray chamber
255 operating at room temperature). The nebulizer gas flow rate employed for the conventional
256 system was 0.4 L min^{-1} . Table 2 shows that h-TISIS readouts were up to 13 fold improved as
257 compared to those of the cyclonic spray chamber. Limits of detection (LODs) were determined
258 according to the $3s_b$ criterion, where s_b was the standard deviation of ten consecutive blank
259 measurements. As expected from the sensitivity data, the highest LODs (Table 2) were obtained
260 for the conventional sample introduction system. It is however important to note that the

261 discrepancies observed across the trends in LODs and the analytical readouts are attributed to
262 the dependence of the spray chamber design upon the standard deviation of the background.

263

264 *System configuration and evaluation of the analytical protocol*

265 Our experimental setup features significant advances as compared to previous works in the field
266 of LIS.^{20,21} For example, the induction of solvent dispersion by stirring bar rotation did not
267 require any additional “driving device” to generate a rotating magnetic field as reported
268 previously.^{20,21} As the syringe pump was placed here in common up-right orientation, the
269 magnetic stirring bar had to move with the piston so that the motor was fixed to the piston bar to
270 assure steady leveling of both motor and stirrer. To reach the required rotation rate of 800 rpm
271 for solvent dispersion, the stirring bar had to turn smoothly inside the syringe. A 15 × 4 mm
272 stirring bar was thus sandpapered to a 14 mm length (syringe inner diameter was 14.5 mm).
273 Smaller stirring bars (e.g. 10 mm × 2 mm), potentially offering a lower dead volume, were not
274 able to keep up with the required rotation rate but dangle inside the syringe. Due to the inertia of
275 the liquid, the stirring bar is slowed down at the onset of stirring. Thus, a purpose-made control
276 circuit was used for a slow turn-on of the inducing motor.²⁰ The motor then reached its final
277 speed after approximately 5 s, which enabled synchronized rotation of the stirring bar.

278 Regarding the analytical protocol for in-syringe DLLME, the following two operational
279 sequences for in-line sequential aspiration of solutions to the syringe were tested: 1: Air,
280 extraction solvent, sample, air, DDTP reagent and air; and, 2: Air, sample, air, DDTP reagent,
281 extraction solvent and air. The segmentation between the sample and the DDTP reagent was
282 done to prevent complex formation already inside the holding coil and the potential sorption of
283 the chelate onto the hydrophobic walls of the flow manifold, which would in turn jeopardize the
284 precision and the analyte recovery and lead to carry-over effects. Air was further found to favor
285 vortex formation with the consequent dispersion of the extraction solvent into tiny droplets. It
286 was demonstrated that the first aspiration sequence was superior in terms of peak height (1.4-1.5
287 times higher signal) and thus was kept further on. Because the extraction solvent was the first

288 solution introduced into the syringe, smaller droplets were formed, thus enhancing the surface
289 area with the subsequent improvement of the extraction efficiency.

290 One disadvantage of the LIS-based extraction system herein proposed is the potential cross-over
291 contamination because of the syringe void volume caused by the stirring bar along with the
292 possibility of sorption of organic phase droplets onto the PTFE bar. Generally, the rinsing of the
293 syringe after extraction is done in three steps; a first cleaning step with isopropanol, to remove
294 organic solvent remnants; a second step with a concentration of nitric acid ranging from 2-15%
295 (v/v) to remove metal leftovers and, finally, with the sample, in order to rinse the system with
296 the sample matrix itself. However, the hydrophobic analyte complexes can further be retained in
297 the tubing and injection valve, potentially leading to carry-over effects. To evaluate the
298 effectiveness of several cleaning protocols (see Table S3), the concentrations of metals in three
299 consecutive blank samples analyzed after a standard of $100 \mu\text{g L}^{-1}$ of Ag, Cd, Cu, and Pb were
300 determined. Figure S3 shows the percentage of the Ag blank signals in consecutive injections
301 with respect to that obtained at the $100 \mu\text{g L}^{-1}$ level. The rinsing protocol capitalizing upon 15%
302 (v/v) HNO_3 provided the best performance because signals for the first extraction of the blank
303 corresponded to only 5% of the signal obtained for the $100 \mu\text{g L}^{-1}$ standard. Similar results were
304 found for Cd, Cu and Pb. In the remainder of washing protocols using 2-10% (v/v) HNO_3 , the
305 first blank signal amounted to as much as ca 20-95% of the initial Ag signal.

306

307 *Selection of physical and chemical parameters*

308 *Volume of the extraction solvent, DDTP concentration and extraction time*

309 The volume of the extraction solvent in the automatic LIS procedure is particularly important
310 inasmuch as large volumes facilitate quantitative extraction efficiency while microvolumes
311 (usually a few microliters) are preferable with respect to the improvement of preconcentration
312 factors. Evaluation of the volume of xylene as extraction solvent was performed by comparison
313 of the analytical readouts obtained for volumes in the range of 220 to 320 μL at the $100 \mu\text{g L}^{-1}$

314 level. Larger solvent volumes were considered unacceptable for analyte enrichment while
315 smaller volumes of solvent were unlikely to be applicable herein as the system's reliability is
316 based on the premise that the solvent droplets coalesce to one phase so that introduction of
317 droplets of the aqueous phase into the h-TISIS-ICP OES is circumvented. The ICP OES signals
318 were normalized with respect to the maximum peak height (obtained with 270 μL). Figure S4
319 indicates that the normalized readouts increased with the volume of extraction solvent up to 270
320 μL , with repeatabilities in all instances better than 3%. Similar trends were found for peak area;
321 hence, the analytical signal was taken as peak height throughout. Note that similar behavior was
322 found for all the elements, therefore, Ag and Cd were selected as model analytes for further
323 studies.

324 In DLLME, the higher the interfacial area between immiscible phases is the shorter the
325 extraction time for attaining comparable extraction efficiencies. For a fixed stirring rate (*viz.*,
326 800 rpm), the effect of the stirring time was evaluated. The minimum extraction time to achieve
327 pseudo-equilibrium conditions was estimated at the onset of the curvature of the regression line
328 of the peak height against extraction time for which the analytical readouts approach to steady-
329 state conditions. The pseudo-equilibrium conditions were reached at 60-65 s for all the elements
330 under the experimental conditions indicated above. Moreover, it was observed that almost 100%
331 (in absolute mass) of the analytes were extracted in the organic phase for stirring times of 100-
332 120 s. For stirring times >100 s the influence of the extraction time was virtually negligible as
333 the peak height remained practically unaltered. However, the intra-day precision improved with
334 the extraction time, reaching RSD values lower than 5% at 120 s. An extraction time of 120 s
335 was therefore chosen for the remaining work. The concentration of the extraction agent was also
336 evaluated. Figure S5 indicates that peak heights increased with DDTP concentration up to 50
337 mmol L^{-1} , which was selected for the remainder of the experiments.

338

339 *Effect of the acid and counter ion on the extraction procedure*

340 The effect of the acid nature and counter ions on the extraction efficiency of target metals was
341 evaluated. Hence, a cohort of six standards was prepared with the same metal concentration but
342 with increasing concentrations of strong acids (HCl or HNO₃) to evaluate the potential salting-
343 out effects and metal complexation. The matrix composition was: 0.21, 0.51 or 1.03 mol L⁻¹ in
344 HNO₃ or HCl. According to previous researchers,²¹ the effect of the two counter anions as
345 interfering species for DDTP extraction was not statistically significant (Fig. S6). With respect
346 to the acidity of the sample matrix, a loss of signal intensity was observed at the concentration
347 level of 1.03 mol L⁻¹ regardless of the acid nature. For nitric acid, 6% and 12 % signal losses
348 were observed for Ag and Cu, respectively. On the other hand, a 7% loss of peak height was
349 observed in both cases for 1.03 mol L⁻¹ HCl.

350

351 *Analytical method performance*

352 Under the selected experimental conditions, a linear correlation of peak height against analyte
353 concentration in aqueous medium subjected to automatic DLLME was observed. The
354 calibration was performed using six concentration levels in aqueous phase from 0.4 up to 11 µg
355 L⁻¹ with an injection volume of 12 µL of organic phase. Coefficients of determination (R²)
356 higher than 0.9991 were obtained for five inter-day calibration curves. As a benchmark of inter-
357 day precision, relative standard deviations were 5, 7, 4, and 8 % for the slopes of the calibration
358 curves of Ag, Cd, Cu, and Pb, respectively. Moreover, no outlying measurements (> three times
359 the standard error of the slope) were found. LODs were calculated according to the 3s_b criterion
360 (n=10), and in all instances were lower than 0.1 µg L⁻¹. LOQs were 0.16, 0.14, 0.14 and 0.21 µg
361 L⁻¹ for Ag, Cd, Cu, and Pb, respectively. Repeatability values for six consecutive analysis of a
362 2.0 µg L⁻¹ aqueous standard were 3.1, 4.0, 2.8 and 3.9 % for Ag, Cd, Cu and Pb, respectively.

363 An alternative calibration method was also tested. In this case, organic standards (12 µL) were
364 introduced directly to the ICP OES following the air-segmented injection methodology
365 described above. Organic standards were prepared using xylene as a diluent of the certified

366 reference material Conostan[®] S-21. Coefficients of determination (R^2) higher than 0.9993 were
367 obtained for five calibration curves within the concentration range spanning from 5-170 $\mu\text{g/L}$ on
368 5 subsequent days. The inter-day precision in terms of sensitivity was similar to that of the
369 procedure with aqueous standards followed by DLLME. Notwithstanding the deterioration in
370 sensitivity (see Table 3) as the organic standards in this second external calibration method are
371 not subjected to preconcentration, LOQs were not proportionally increased because of the
372 deterioration of the blank repeatability values for the LIS-DLLE method. Repeatability values
373 for six consecutive analysis of a 25 $\mu\text{g L}^{-1}$ organic standard were were 2.1, 3.4, 2.7 and 4.2 %
374 for Ag, Cd, Cu and Pb, respectively.

375 The preconcentration factor was obtained as the ratio of the slope of the straight line regression
376 following the automatic LIS extraction procedure to that obtained by direct injection of organic
377 standards into h-TISIS-ICP OES. Table 3 compiles the sensitivities of both calibration curves.
378 The nominal pre-concentration factor was estimated from the ratio of the sample volume (3.60
379 mL) to that of the organic solvent (270 μL), that is, 13.3. Table 3 shows that the experimentally
380 obtained pre-concentration factors were similar to the nominal value, thus signalling that the
381 extraction efficiency for all the metals was close to 100%.

382 The entire automatic LIS procedure, including mixing of the sample and reagents, extraction,
383 phase separation, measurement and system cleaning, lasted ca. 375 s, which gives rise to a
384 sample throughput of 9 h^{-1} . The cleaning protocol using 1.2 mL of isopropanol lasted 15 s.
385 Shortening of the rinsing time could most likely be effected by replacing the rotary valve by a
386 low-dead volume stainless steel stator and rotor so as to minimize carry-over effects.

387

388 *Analysis of real samples*

389 With the aim of validating the extraction methodology, five real samples including seawater,
390 salt, salt without sodium, grape juice and apple juice were analyzed by LIS-DLLME. To this
391 end, a given aliquot was spiked with 2.0 $\mu\text{g L}^{-1}$ of a multi-elemental solution in the aqueous
392 phase. Consequently, the analytical concentration in the organic phase after the preconcentration

393 step was around $25 \mu\text{g L}^{-1}$. Note that the non-spiked samples were also analyzed. Original metal
394 concentrations are summarized in Table S4.

395 Table 4 (right) lists the relative recoveries for Ag, Cd, Cu and Pb, which were close to 100% in
396 all the cases. It can therefore be concluded that additive or multiplicative matrix effects for any
397 of the tested samples, even for typically not applicable samples of high salt content, were
398 insignificant. Recovery values were also calculated using a calibration curve obtained by direct
399 injection of the organic standards into the ICP (see Table 4 left). In this case, the concentration
400 of the organic standards was divided by the preconcentration factor and used as X-axis data with
401 the ICP OES readouts as Y-axis for direct analysis of the spike recoveries in the aqueous phase.
402 Experimental results compiled in Table 4 demonstrated that both external calibration methods
403 provide comparable metal recoveries for all the samples with troublesome matrices. It is
404 important to point out that there is no need to subject the aqueous standards to the DLLME
405 procedure to get reliable results as the target metals regardless of the matrix composition were
406 quantitatively extracted in the organic phase.

407 For further QC/QA assessment, two serum reference materials, differentiated by the level of
408 metal concentration, were analyzed by LIS-DLLME. For further QC/QA assessment, two serum
409 certified reference materials (CRM), differentiated by the level of metal concentration, were
410 analyzed by LIS-DLLME. Statistical assessment of experimental data for the CRMs was
411 done by comparison of the difference between the certified and the measured values
412 against the associated expanded uncertainty (U_{Δ}) because the number of accepted sets of
413 data is not provided in the CRM report. The absolute difference (Δ_m) between the mean
414 measured value (c_m) and the mean certified value (c_{CRM}) is calculated according to
415 equation 1. The combined uncertainty (u_{Δ}) was calculated, based on equation 2, from
416 the uncertainty of the certified value (u_{CRM}) and the standard deviation (s_m) of the
417 experimental data. The expanded uncertainty U_{Δ} for a confidence level of
418 approximately 95 % is obtained by multiplying the combined uncertainty (u_{Δ}) by a

419 coverage factor (k) equal to 2 (Equation 3). To evaluate the method performance, Δ_m
420 was compared against U_Δ . Because Δ_m is in all cases $< U_\Delta$, no statistically significant
421 differences were found at the 95% level between the values obtained experimentally and
422 the certified concentrations for any of the target elements (see Table 5 and Table S5).

423

$$424 \quad \Delta_m = |c_m - c_{CRM}| \quad \text{Equation 1}$$

$$425 \quad u_\Delta = \sqrt{s_m^2 + u_{CRM}^2} \quad \text{Equation 2}$$

$$426 \quad U_\Delta = k u_\Delta \quad \text{Equation 3}$$

427

428

429 **Conclusions**

430 In this work, a novel approach capitalizing on a portable flow setup has been proposed for the
431 first time for the coupling of automatic in-syringe magnetic stirring-assisted dispersive liquid-
432 liquid microextraction to ICP spectrometry for direct analysis of metal laden organic extracts
433 using an h-TISIS-based total sample consumption system. With this miniaturized sample
434 introduction system, negligible matrix effects were observed in the analysis of carbon-
435 containing matrixes. Because of the high stability constants of DDTP-metal chelates, back-
436 extraction to aqueous phase for conventional ICP measurements in the aqueous phase is proven
437 unfeasible. Using a univariate optimization strategy suitable experimental conditions were
438 found for DLLME-h-TISIS-ICP OES detection of trace level concentrations of target elements
439 in troublesome samples with enrichment factors of ca. 13. Limits of detection found for two
440 distinct calibration procedures were: 0.05, 0.04, 0.04 and 0.06 $\mu\text{g L}^{-1}$ for Ag, Cd, Cu and Pb
441 (extraction procedure) and 0.07, 0.09, 0.06 and 0.10 $\mu\text{g L}^{-1}$ for Ag, Cd, Cu and Pb (direct
442 injection of standards) respectively, allowing its successful application to the analysis of
443 certified serum materials and spiked environmental samples and beverages. Efficiencies of

444 extraction were close to 100 % with repeatabilities usually down to 8%. Therefore, external
445 calibration can be streamlined by direct injection of organic standards into the h-TISIS-ICP
446 detector system with no need to subject them to the extraction procedure. Further work is
447 underway to expand the scope of the hyphenated LIS-DLLME-h-TISIS-ICP system for
448 detection of bioaccessible metals, metalloids and organometallic compounds in complex
449 foodstuff and soil extracts.

450

451 **Supplementary Information.** Additional experimental data and information includes
452 (i) Images of the flow setup and plasma characteristics, (ii) Readouts of cleaning
453 procedures and operational steps, (iii) Effect of volume of organic phase on the
454 analytical readouts, (iv) Effect of chelating reagent concentration on the analytical
455 readouts, (v) Effect of acid type and concentration on the analytical readouts, (vi)
456 Detailed analytical procedure and cleansing protocol, (vii) Concentration of targeted
457 species in the real samples and (viii) Statistical analysis of experimental data for CRM.

458

459 **Acknowledgements**

460 B. Horstkotte acknowledges the financial support by an ERASMUS+ scholarship No XIII / 3/
461 15-16 and by the Czech Science Foundation (project no. P206/15/10781S). K. Fikarová is
462 thankful for an Erasmus student scholarship and financial support of the Charles University
463 (Project SVV 260 292/2016). M. Miró acknowledges financial support from the Spanish State
464 Research Agency through projects CTM2014-56628-C3-3-R (AEI/FEDER, UE) and
465 CTM2014-61553-EXP (AEI/FEDER, UE).

466

467 **Table 1. Operating conditions of the ICP OES furnished with h-TISIS for injection of**
 468 **organic samples**

Variable	Value
Injected sample volume [μL]	12
Nebulizer gas flow, Q_g [L min^{-1}]	0.26
Outer gas flow [L min^{-1}]	15
Intermediate gas flow [L min^{-1}]	1.0
Rf power [kW]	1.35
Integration time [ms]	25
Sampling time [s]	1
Plasma viewing mode]	Axial
Temperature spray chamber [$^{\circ}\text{C}$]	350
Elements and Wavelengths [nm]	Ag 328.068
	Cd 228.802
	Cu 324.752
	Pb 220.353

469

470

471 **Table 2. Peak height and LODs obtained for the h-TISIS compared against those obtained**
 472 **for the conventional system.***

	h-TISIS ^Φ			Conventional system ^Φ			Peak height ^(h-TISIS) / Peak height ^(Conventional)	LOD ^(Conventional) / LOD ^(hTISIS)
	Peak height	RSD (%)	LOD (μg L ⁻¹)	Peak height	RSD (%)	LOD (μg L ⁻¹)		
Ag	6.1×10 ⁵	2.4	0.6	5.0×10 ⁴	11.2	2.3	12	4
Cd	1.4×10 ⁴	7.2	0.4	1.3×10 ³	9.5	3.6	11	10
Cu	8.1×10 ⁵	2.7	0.5	6.1×10 ⁴	1.6	1.9	13	4
Pb	1.4×10 ⁴	4.6	0.4	1.4×10 ³	10.3	2.1	10	5

473 * Metal concentration: 100 μg L⁻¹ in xylene. Injected volume: 12 μL. Q_g (h-TISIS): 0.26 L min⁻¹, Q_g
 474 (Conventional system): 0.40 L min⁻¹.
 475 ^Φ 10 replicates.

476

477 **Table 3. Slopes of the calibration curves by the automatic LIS-DLLME procedure and the**
 478 **direct injection of organic standards along with the experimental pre-concentration**
 479 **factors**

	Slope – Aqueous standards - LIS-DLLME procedure (L µg⁻¹)	Slope – Organic standards - Direct injection (L µg⁻¹)	Pre-concentration factor
Ag	1.1×10 ⁵	8.1×10 ³	13.6
Cd	1.7×10 ³	0.13×10 ³	13.1
Cu	7.9×10 ⁴	5.9×10 ³	13.4
Pb	1.9×10 ³	0.14×10 ³	13.5

480

481

Table 4. Relative recoveries (%) for complex samples using the LIS-DLME-h-TISIS-ICP OES system

Samples	<i>Standards: Direct injection*</i>								<i>Standards: Extraction procedure#</i>							
	Ag		Cd		Cu		Pb		Ag		Cd		Cu		Pb	
	Mean	RSD (%)	Mean	RSD (%)	Mean	RSD (%)	Mean	RSD (%)	Mean	RSD (%)	Mean	RSD (%)	Mean	RSD (%)	Mean	RSD (%)
<i>Seawater</i>	94	1.4	96	1.1	103	0.5	95	0.6	95	1.4	97	1.1	103	0.5	96	0.6
<i>Salt A</i>	98	1.1	99	0.6	95	0.2	94	0.3	99	1.1	100	0.6	97	0.2	95	0.3
<i>Salt B (Without Na)</i>	96	1.2	98	1.1	96	1.1	93	2.0	97	1.2	100	1.1	97	1.1	94	2.0
<i>Apple juice</i>	98	0.9	95	1.1	97	1.2	94	1.0	99	0.9	96	1.0	98	1.2	96	1.0
<i>Grape juice</i>	97	0.3	92	2.0	97	1.1	97	0.7	97	0.3	93	2.0	98	1.1	98	0.7

* The standards were prepared in xylene and directly injected in triplicate into the h-TISIS-ICP OES without the use of the extraction procedure.

The standards were prepared in Ultrapure water, then analyte extraction was performed into xylene (in triplicate) and, finally, a small volume of each extract (in triplicate) was injected into the h-TISIS-ICP OES

Table 5. Concentrations for the reconstituted certified serum samples as obtained by the automatic LIS-DLLME procedure

	Serum - Level I						Serum - Level II ^Φ					
	Ag		Cd		Cu		Ag		Cd		Cu	
	Mean ($\mu\text{g L}^{-1}$)	s ($\mu\text{g L}^{-1}$)	Mean ($\mu\text{g L}^{-1}$)	s ($\mu\text{g L}^{-1}$)	Mean ($\mu\text{g L}^{-1}$)	s ($\mu\text{g L}^{-1}$)	Mean ($\mu\text{g L}^{-1}$)	s ($\mu\text{g L}^{-1}$)	Mean ($\mu\text{g L}^{-1}$)	s ($\mu\text{g L}^{-1}$)	Mean ($\mu\text{g L}^{-1}$)	s ($\mu\text{g L}^{-1}$)
Extraction procedure*	9.29 [¥]	0.09	2.2 [¥]	0.01	0.775 [¥]	0.002	47.3 ^Φ	0.2	4.62 ^Φ	0.01	1.23 ^Φ	0.01
Direct injection[#]	9.49	0.09	2.2	0.02	0.781	0.003	47.5	0.2	4.63	0.01	1.22	0.02
Certified value*	9.85	2.00	2.28	0.47	0.801	0.122	48.0	9.8	4.54	0.93	1.34	0.20

*The standards were prepared in Ultrapure water, and analyte extraction was performed into xylene (in triplicate). A small volume of the extract (in triplicate) was injected into the h-TISIS-ICP OES.

[¥] The calibration was performed using seven concentration levels of aqueous standards ranging from 0.3 up to 11 $\mu\text{g L}^{-1}$.

^Φ The calibration was performed using eight concentration levels of aqueous standards ranging from 1 up to 15 $\mu\text{g L}^{-1}$. For Ag determination, the sample was 1:4 diluted with Ultrapure water.

[#] The standards were prepared in xylene and directly injected in triplicate into the h-TISIS-ICP OES without applying the extraction procedure. The calibration was performed using ten concentration levels of organic standards ranging from 0.5 up to 170 $\mu\text{g L}^{-1}$.

* The standard deviation was estimated as the combined standard uncertainty with a coverage factor of 1.96 at the 95% confidence level.

Figure captions

Figure 1. Outline of the automatic and miniaturized LIS-DLLME system. HV – Head valve (of syringe, positions IN, OUT, and TOP), IV – Injection valve, IL – Injection loop, 8 cm, 0.25 mm i.d., M – DC motor, PP – Peristaltic pump, SP – Syringe pump, SV – Selection valve. Tube dimensions: A – 5 cm, 0.8 mm i.d., B – 15 cm, 1.0 mm i.d., C – Transfer line 20 cm, 0.5 mm i.d., E – 20 cm, 0.25 mm i.d. (PEEK), F – red-orange peristaltic/elastic tube, 40 cm, 0.16 mm i.d., G – Magnetic stirring bar.

Figure 2. Normalized peak height with respect of that obtained at room temperature for different analytes and h-TISIS temperatures. Metal concentration: $100 \mu\text{g L}^{-1}$. Injected volume: $12 \mu\text{L}$ xylene. Q_g : 0.26 L min^{-1} .

Figure 1


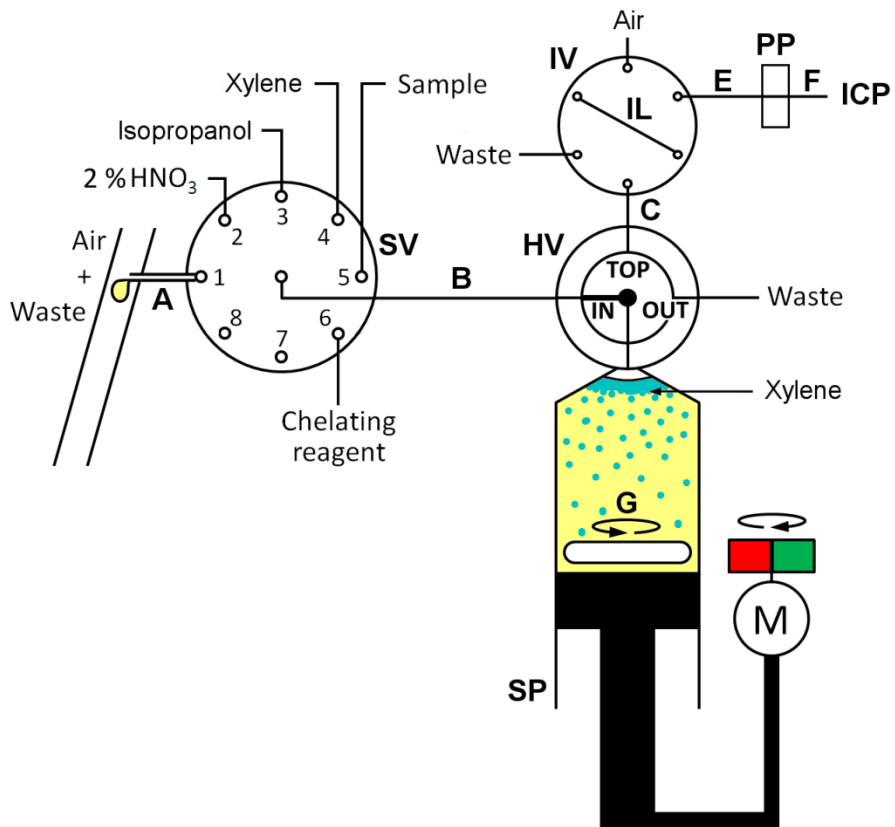


Figure 2

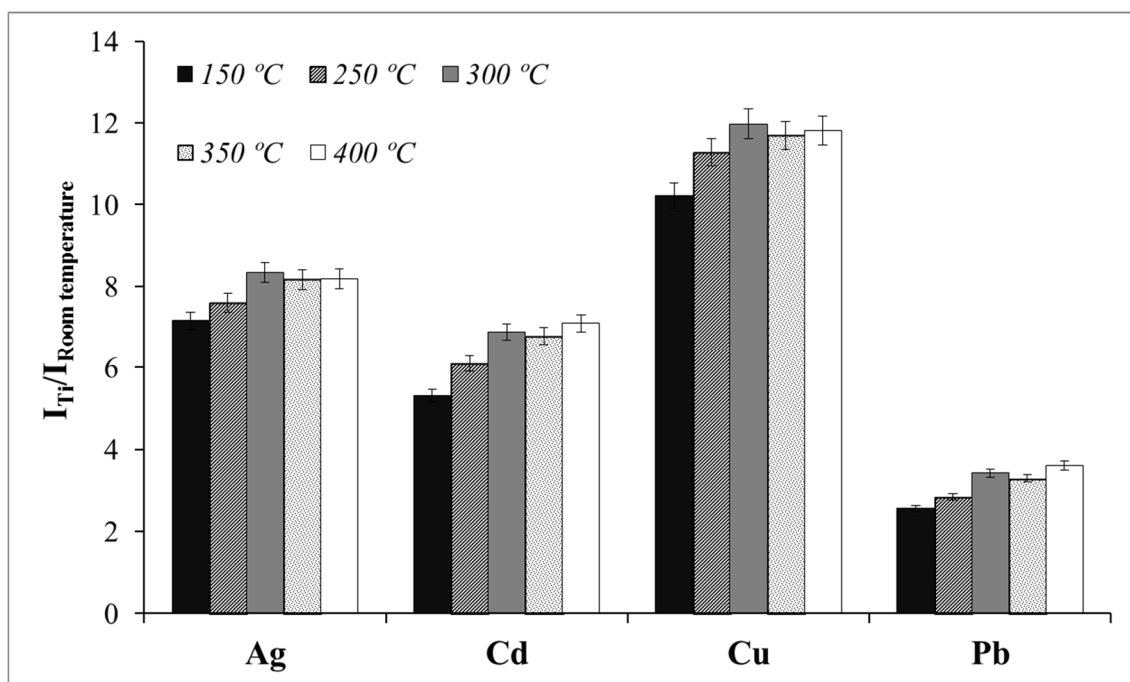

References

- ¹Wang, J.; Hansen, E.H.; *Anal. Chim. Acta*, **2002**, 456, 283-292.
- ²Hansen, E.H.; *J. Environ. Sci. Health A Tox. Hazard. Subst. Environ. Eng.*, **2005**, 40, 1507-1524.
- ³Miró, M.; Hansen, E.H.; *Anal. Chim. Acta*, **2013**, 782, 1-11.
- ⁴Leclercq, A.; Nonell, A.; Todolí, J.L.; Bresson, C.; Vio, L.; Vercouter, T.; Chartier, F.; *Anal. Chim. Acta*, **2015**, 885, 33-56.
- ⁵Leclercq, A.; Nonell, A.; Todolí, J.L.; Bresson, C.; Vio, L.; Vercouter, T.; Chartier, F.; *Anal. Chim. Acta*, **2015**, 885, 57-91.
- ⁶El-Shahawi, M.S.; Al-Saidi, H.M.; *TrAC-Trends Anal. Chem.*, **2013**, 44, 12-24.
- ⁷Andruch, V.; Balogh, I.S.; Kocurova, L.; Šandrejová, J.; *J. Anal. At. Spectrom.*, **2013**, 28, 19-32.
- ⁸Satyanarayanan, M.; Balaram, V.; Rao, T.G.; Dasaram, B.; Ramesh, S.L.; Mathur, R., Drolia, R.K.; *Indian J. Mar. Sci.*, **2007**, 36, 71-75.
- ⁹Jia, X.; Han, Y.; Liu, X.; Duan, T.; Chen, H.; *Microchim. Acta*, **2010**, 171, 49-56.
- ¹⁰Mallah, M.H.; Shemirani, F.; Maragheh, M.G.; *J. Radioanal. Nucl. Chem.*, **2008**, 278, 97-102.
- ¹¹Sereshti, H.; Heravi, Y.E.; Samadi, S.; *Talanta*, **2012**, 97, 235-241.
- ¹²Fang, Z.L.; *Flow-injection separation and preconcentration*, VCH-Weinheim, 1993.
- ¹³Wang, J.; Hansen, E.H.; *J. Anal. At. Spectrom.*, **2002**, 17, 1284-1289.
- ¹⁴Sánchez, R.; Todolí, J.L.; Lienemann, C.P.; Mermet, J.M.; *J. Anal. At. Spectrom.*, **2012**, 27, 937-945.
- ¹⁵Ardini, F.; Grotti, M.; Sánchez, R.; Todolí, J.L.; *J. Anal. At. Spectrom.*, **2012**, 27, 1400-1404.
- ¹⁶Maya, F.; Horstkotte, B.; Estela, J.M.; Cerdà, V.; *TrAC-Trends Anal. Chem.*, **2014**, 59, 1-8.

- ¹⁷Maya,F.;Horstkotte,B.;Estela,J.M.;Cerdà,V.; *Anal. Bioanal. Chem.*,**2012**,*404*, 909-917.
- ¹⁸Růžicka, J.;Marshall,G.D.;*Anal. Chim. Acta*,**1990**,*237*,329-343.
- ¹⁹Hansen,E.H.;Miró, M.;*TrAC-Trends Anal.Chem.*,**2007**,*26*,18-26.
- ²⁰Horstkotte,B.;Suárez,R.;Solich,P.;Cerdà,V.; *Anal. Chim. Acta*,**2013**,*788*, 52-60.
- ²¹Suárez,R.;Horstkotte,B.;Cerdà,V.; *Talanta*,**2014**,*130*, 555-560.
- ²²Al-Saidi,H.M.;Emara,A.A.A.; *J. Saudi Chem. Soc.*,**2014**,*18*,745-761.
- ²³Mitani,C.;Anthemidis,A.N.; *Curr Anal. Chem.*,**2013**, *9*,250-278.
- ²⁴Alexovič,M.;Horstkotte,B.,Solich, P.;Sabo,J.; *Anal. Chim. Acta*,**2016**,*906*, 22-40.
- ²⁵Alexovič,M.;Horstkotte,B.,Solich, P.;Sabo,J.; *Anal. Chim. Acta*,**2016**,*907*, 18-30.
- ²⁶Giordano,B.C.;Burgi,D.S.;Hart,S.J.;Terray,A.; *Anal. Chim. Acta*,**2012**,*718*, 11-24.
- ²⁷Verboket,P.E.;Borovinskaya,O.;Meyer,N.;Günther,D.;Dittrich,P.S.;*Anal. Chem.*,**2014**, *86*,6012-6018.
- ²⁸Miró,M.;Estela,J.M.;Cerdà,V.; *Curr. Anal. Chem.*,**2005**, *1*,329-343.
- ²⁹Anthemidis,A.N.;Miró,M.; *Appl. Spectr. Rev.*,**2009**, *44*,140–167.
- ³⁰Silvestre,C.I.C.;Santosa,J.L.M.; Lima,J.L.F.C.;Zagatto, E.A.G.;*Anal.Chim.Acta*, **2009**, *652*, 54-65.
- ³¹Giakisikli,G.G.;Miró, M.;Anthemidis,A.N.; *Anal. Chem.*,**2013**, *85*, 8968-8972.
- ³²Mitani, C.; Kotzamanidou, A.; Anthemidis, A.N.; *J. Anal. At. Spectrom.*,**2014**, *29*, 1491-1498.
- ³³Giakisikli,G.G.;Anthemidis,A.N.;*Talanta, Talanta*, **2017**,*166*, 364-368.
- ³⁴Ramos,J.C.;Curtius,A.J.;Borges,D.L.G.; *Appl. Spectr. Rev.*, **2012**, *47*,583-619.
- ³⁵Ramos,J.C.;Borges,D.L.G.; *J. Anal. At. Spectrom.*,**2014**, *29*,304-314.
- ³⁶Dittert,I.M.;Vitali,L.;Chaves,E.S.;Maranhão,T.A.;Borges,D.L.G.,deFávere,V.T.; Curtius, A.J.; *Anal. Methods*,**2014**, *6*, 5584-5589.

³⁷Cocovi-Solberg,D.J.; Miró,M.; *Anal. Bioanal. Chem.*,**2015**, 407,6227-6233.

³⁸Todolí,J.L.;Mermet,J.M.; *J. Anal. At. Spectrom.*,**2003**, 18,1185-1191.